


$\times 10^6$

### Phase tracker calibration – X arm

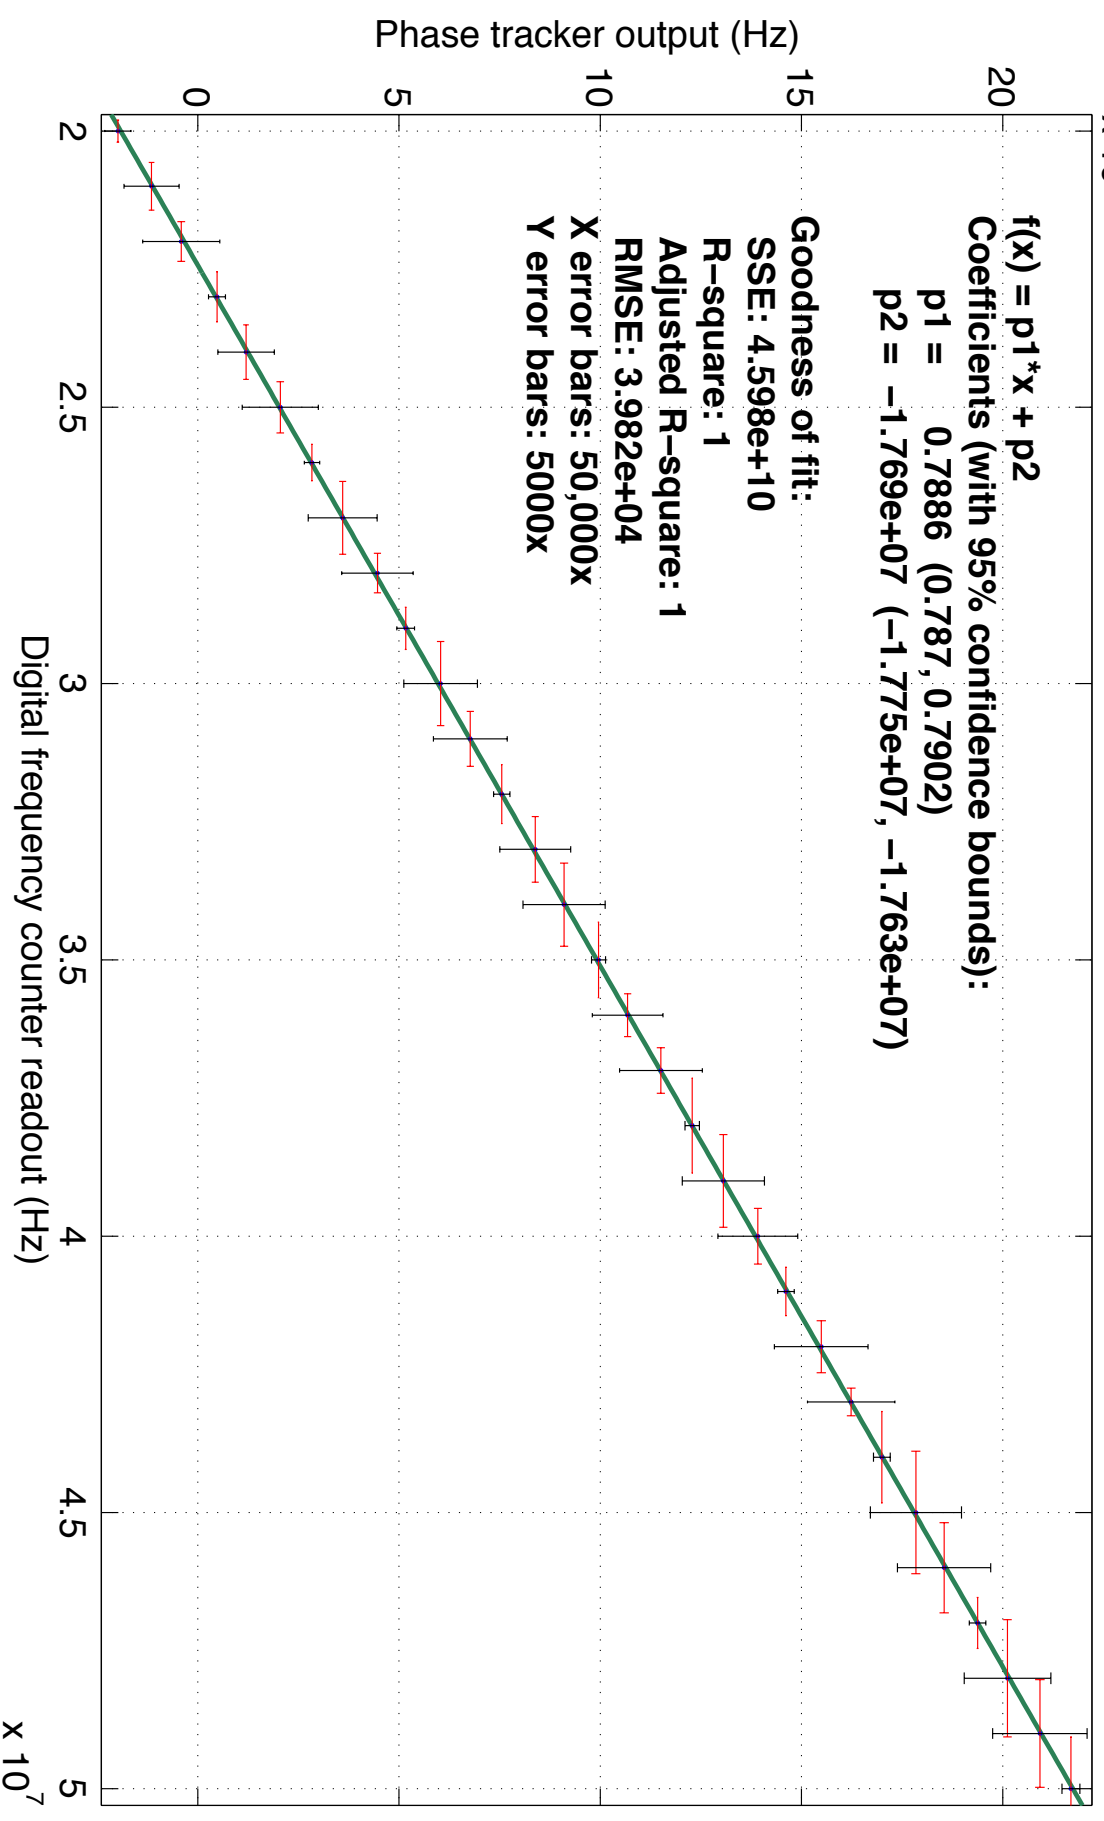

$\times 10^7$