


PRM OSEM sensing electronics (with tester box)

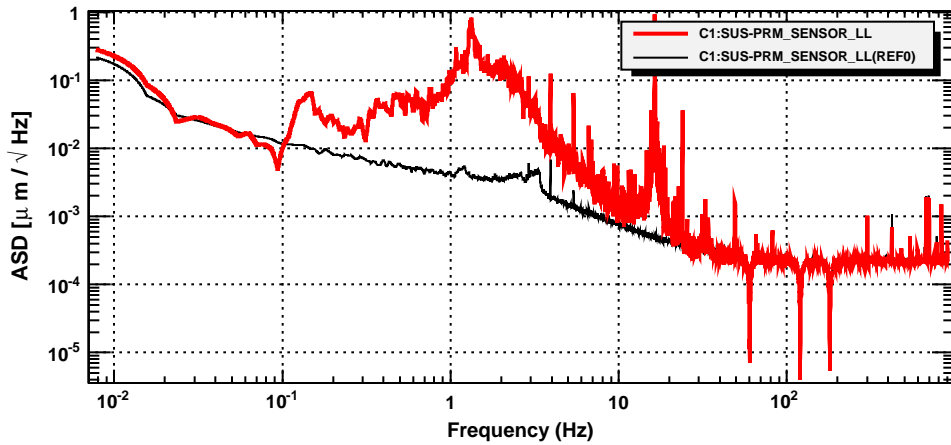


*T0=31/10/2019 05:04:18

*Avg=6/Bin=11L

BW=0.0117178

SIDE

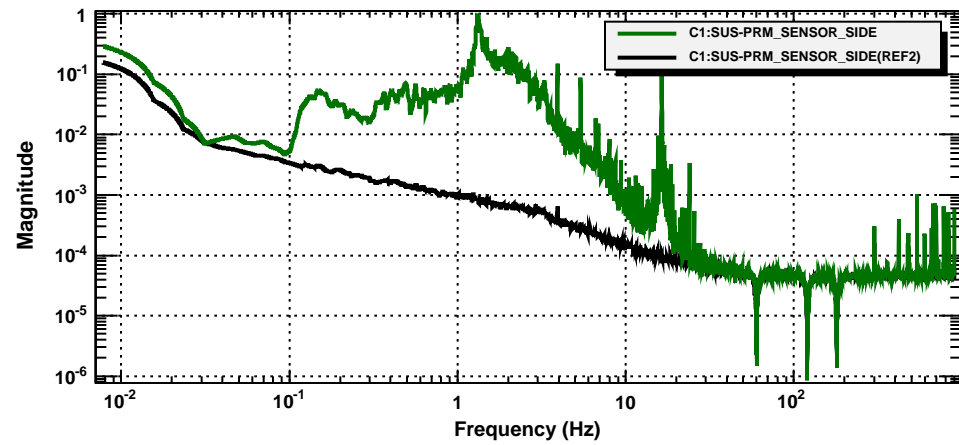


*T0=31/10/2019 05:04:18

*Avg=6/Bin=11L

BW=0.0117178

UR

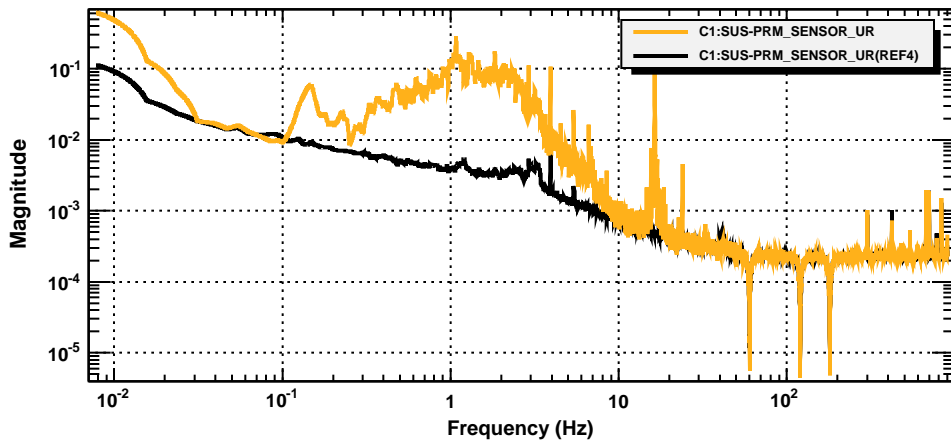


*T0=31/10/2019 05:04:18

*Avg=6/Bin=11L

BW=0.0117178

LR

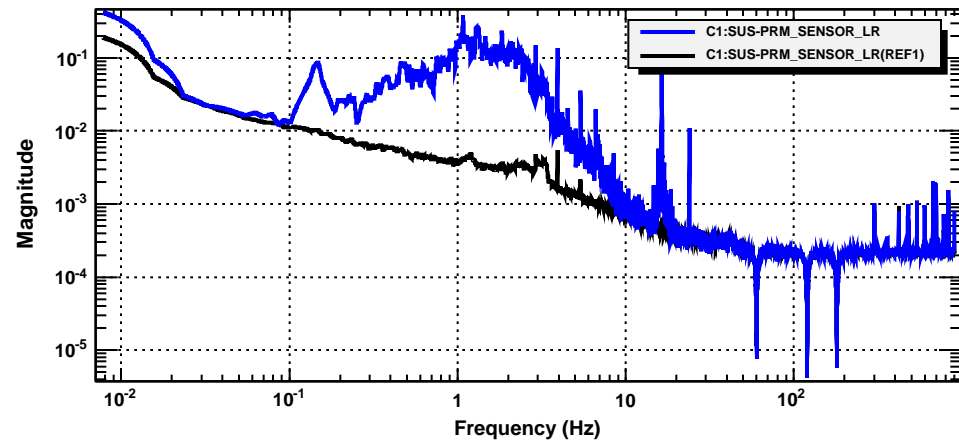


*T0=31/10/2019 05:04:18

*Avg=6/Bin=11L

BW=0.0117178

UL

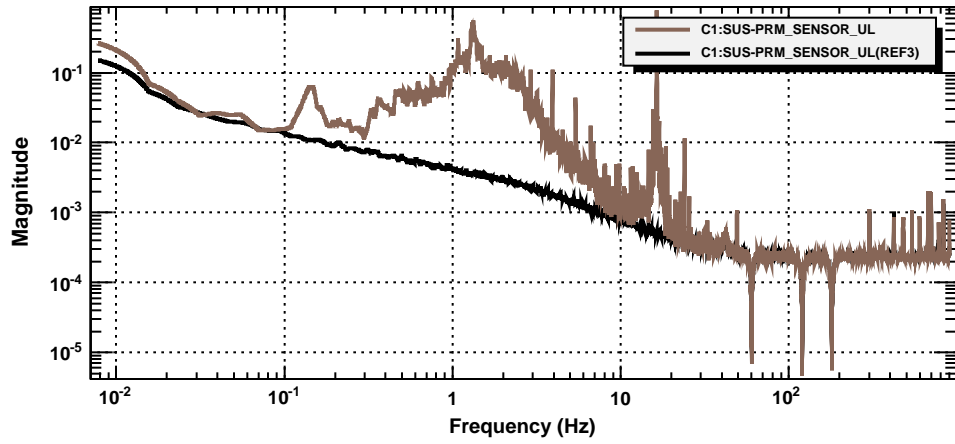

*T0=31/10/2019 05:04:18

*Avg=6/Bin=11L

BW=0.0117178